



中国认可  
国际互认  
检测  
TESTING  
CNAS L5772

# Test Report

## Test Requirement:

According to the requirement of the Module C2 (SPC CE-062\_EN M5 PPE ) of Applus+, the test item(s) of the sample is according to the standard EN149:2001+A1:2009.

**Product Name:** Filtering Half Mask

**Report No.:** PTC21030502102C-EN01

**APPLUS +With ID number:** 21/32302024

**Client:** Mezorison Health Science & Technology (Shenzhen) Co.,Ltd.

**Client Address:** No.12 Yuhe Road, Shiyan Town, Baoan District, Shenzhen

**Manufacturer:** Mezorison Health Science & Technology (Shenzhen) Co.,Ltd.

**Manufacturer Address:** 2nd floor, Gaoke building, No.8 Tangkeng Rd, Shiyan, Baoan district, Shenzhen, China

**Contact:** Mr. Chen Ping

**Model(s):** MZC-KZ(S)

**Classification:** FFP2 NR

**Date of Tests:** 2021.04.26~2021.04.30

Signed for and on Behalf of PTC

Prepare by:

Checked by:

Approved by:

Anne

Jue

Jim Mo



This report is issued according to the general clauses in [www.ptc-testing.com](http://www.ptc-testing.com) by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted.  
The report could not be copied without permission

**Precise Testing & Certification (Guangdong) Co., Ltd. (PTC)**

Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.  
Tel: 86-769-38808222 Fax: 86-769-38826111 [http:// www.ptc-testing.com](http://www.ptc-testing.com)



# Test Report

Report No.:PTC21030502102C-EN01

Issue Date:Apr.30, 2021

Page 2 of 13

## Summary of assessment

Clause	Assessment
7.3 Visual inspection	PASS
7.5 Material	PASS
7.9.1 Total inward leakage	PASS
7.9.2 Penetration of filter material	PASS
7.12 Carbon dioxide content of the inhalation air	PASS
7.16 Breathing resistance	PASS
7.18 Demountable parts	N/A

### Remark:

PASS: comply with requirement of standard

N/A: not application

This report is issued according to the general clauses in [www.ptc-testing.com](http://www.ptc-testing.com) by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted.

The report could not be copied without permission

**Precise Testing & Certification (Guangdong) Co., Ltd. (PTC)**

Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.  
Tel: 86-769-38808222 Fax: 86-769-38826111 [http:// www.ptc-testing.com](http://www.ptc-testing.com)



# Test Report

Report No.:PTC21030502102C-EN01

Issue Date:Apr.30, 2021

Page 3 of 13

## Test Result:

Requirement	Test Result	Conclusion
<b>7.3 Visual inspection</b> The visual inspection shall also include the marking and the information supplied by the manufacturer.	Comply	Pass
<b>7.5 Material</b> Materials used shall be suitable to withstand handling and wear over the period for which the particle filtering half mask is designed to be used.  Any material from the filter media released by the air flow through the filter shall not constitute a hazard or nuisance for the wearer.  After undergoing the conditioning described in 8.3.1 none of the particle filtering half masks shall have suffered mechanical failure of the facepiece or straps.  When conditioned in accordance with 8.3.1 and 8.3.2 the particle filtering half mask shall not collapse.	No mechanical failure after undergoing the conditioning described in 8.3.1, No collapse when conditioned in accordance with 8.3.1 and 8.3.2.	Pass
<b>7.9.1 Total inward leakage</b> For particle filtering half masks fitted in accordance with the manufacturer's information, at least 46 out of the 50 individual exercise results (i.e. 10 subjects x 5 exercises) for total inward leakage shall be not greater than 25 % for FFP1, 11 % for FFP2, 5 % for FFP3 and, in addition, at least 8 out of the 10 individual wearer arithmetic means for the total inward leakage shall be not greater than 22 % for FFP1, 8 % for FFP2, 2 % for FFP3.	FFP2, Test results are shown in Annex A Table 7.9.1-A&B	Pass
<b>7.9.2 Penetration of filter material</b> The penetration of the filter of the particle filtering half mask shall meet the requirements of Table 1.	FFP2, Test results are shown in Annex A Table 7.9.2.	Pass

This report is issued according to the general clauses in [www.ptc-testing.com](http://www.ptc-testing.com) by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted.  
The report could not be copied without permission

**Precise Testing & Certification (Guangdong) Co., Ltd. (PTC)**

Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.  
Tel: 86-769-38808222 Fax: 86-769-38826111 <http://www.ptc-testing.com>





# Test Report

Report No.:PTC21030502102C-EN01

Issue Date:Apr.30, 2021

Page 4 of 13

## 7.12 Carbon dioxide content of the inhalation air

The carbon dioxide content of the inhalation air (dead space) shall not exceed an average of 1,0 % (by volume)

Test results are shown in Annex A Table 7.12.

**Pass**

## 7.16 Breathing resistance

Classification	Maximum permitted resistance (mbar)		
	Inhalation		Exhalation
	30 l/min	95 l/min	160 l/min
FFP1	0.6	2.1	3.0
FFP2	0.7	2.4	3.0
FFP3	1.0	3.0	3.0

FFP2. Test results are shown in Annex A Table 7.16.

**Pass**

## 7.18 Demountable parts

All demountable parts (if fitted) shall be readily connected and secured, where possible by hand

No demountable parts.

**N/A**

This report is issued according to the general clauses in [www.ptc-testing.com](http://www.ptc-testing.com) by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted.  
The report could not be copied without permission

**Precise Testing & Certification (Guangdong) Co., Ltd. (PTC)**

Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.  
Tel: 86-769-38808222 Fax: 86-769-38826111 [http:// www.ptc-testing.com](http://www.ptc-testing.com)



# Test Report

Report No.:PTC21030502102C-EN01

Issue Date:Apr.30, 2021

Page 5 of 13

## Annex A: Summarization of Test Data

**Table 7.9.1-A: Inward Leakage Test Data**

Test specification: EN 149:2001+A1:2009 Clause 8.5

Subject	Sample No.	Condition	Walk (%)	Head Side/side (%)	Head up/down (%)	Talk (%)	Walk (%)	Mean (%)
Shi	1	A.R	3.8	4.0	4.4	4.7	4.2	4.2
Li	2	A.R	5.3	5.6	5.5	5.8	5.2	5.5
Liu	3	A.R	4.8	5.0	4.5	5.4	5.3	5.0
Liu	4	A.R	4.2	4.1	4.9	4.9	5.0	4.6
Zhang	5	A.R	4.0	4.9	4.7	4.5	4.2	4.5
Xu	6	T.C	4.7	4.4	4.3	4.5	4.4	4.5
Wu	7	T.C	4.1	4.7	4.3	4.4	4.5	4.4
Yu	8	T.C	4.5	4.5	4.6	4.7	4.8	4.6
Li	9	T.C	3.9	4.3	4.0	4.6	4.4	4.2
Lu	10	T.C	4.3	4.1	3.9	4.0	3.8	4.0

**Table 7.9.1-B: Facial dimension**

Subject	Face Length	Face Width	Face Depth	Mouth Width
Shi	102	127	72	47
Li	100	116	82	51
Liu	101	114	73	47
Liu	104	117	76	46
Zhang	107	123	84	52
Xu	98	120	83	54
Wu	102	113	82	53
Yu	103	117	84	51
Li	103	116	83	48
Lu	102	116	74	52

This report is issued according to the general clauses in [www.ptc-testing.com](http://www.ptc-testing.com) by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted.  
The report could not be copied without permission

**Precise Testing & Certification (Guangdong) Co., Ltd. (PTC)**

Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.  
Tel: 86-769-38808222 Fax: 86-769-38826111 [http:// www.ptc-testing.com](http://www.ptc-testing.com)



# Test Report

Report No.: PTC21030502102C-EN01

Issue Date: Apr.30, 2021

Page 6 of 13

**Table 7.9.2: Penetration of filter material**

Test specification: EN 149:2001+A1:2009 Clause 8.11

Aerosol	Condition	Sample No.	Penetration (%)	Assessment
Sodium chloride test	As received	11	0.4	Pass
		12	0.4	
		13	0.4	
	Simulated wearing treatment	14	0.6	
		15	0.3	
		16	0.2	
	Mechanical strength + Temperature conditioned	17	1.5	
		18	1.5	
		19	1.3	
Paraffin oil test	As received	20	1.3	
		21	1.2	
		22	1.1	
	Simulated wearing treatment	23	1.1	
		24	1.3	
		25	0.7	
	Mechanical strength + Temperature conditioned	26	0.5	
		27	0.6	
		28	1.4	

**Table 7.12: Carbon dioxide content of the inhalation air**

Test specification: EN 149:2001+A1:2009 Clause 8.7

Condition	Sample No.	Result (%)		Assessment
As received	29	0.05	Mean value: 0.05	Pass
	30	0.05		
	31	0.05		

This report is issued according to the general clauses in [www.ptc-testing.com](http://www.ptc-testing.com) by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted.  
The report could not be copied without permission

**Precise Testing & Certification (Guangdong) Co., Ltd. (PTC)**

Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.  
Tel: 86-769-38808222 Fax: 86-769-38826111 [http:// www.ptc-testing.com](http://www.ptc-testing.com)





# Test Report

Report No.: PTC21030502102C-EN01

Issue Date: Apr.30, 2021

Page 7 of 13

**Table 7.16: Breathing resistance (mbar)**

Test specification: EN 149:2001+A1:2009 Clause 8.9

As received	Flow Rate		32					33					34				
	Inhalation	30 l/min	0.51					0.51					0.49				
		95 l/min	1.80					1.75					1.78				
	Exhalation	160 l/min	A	B	C	D	E	A	B	C	D	E	A	B	C	D	E
			2.21	2.22	2.20	2.27	2.26	2.18	2.23	2.19	2.20	2.22	2.24	2.27	2.23	2.27	2.26
Simulated wearing treatment	Flow Rate		35					36					37				
	Inhalation	30 l/min	0.42					0.39					0.39				
		95 l/min	1.48					1.42					1.47				
	Exhalation	160 l/min	A	B	C	D	E	A	B	C	D	E	A	B	C	D	E
			2.03	2.05	2.03	2.02	2.06	2.02	2.01	2.03	2.03	2.00	2.02	2.03	2.03	2.05	2.07
Temperature conditioned	Flow Rate		38					39					40				
	Inhalation	30 l/min	0.39					0.45					0.43				
		95 l/min	1.53					1.56					1.54				
	Exhalation	160 l/min	A	B	C	D	E	A	B	C	D	E	A	B	C	D	E
			1.96	1.95	1.93	1.98	1.94	1.96	1.97	1.98	1.94	1.97	1.93	1.97	1.91	1.91	1.94
Assessment	Pass																

A: Facing directly ahead      B: Facing vertically upwards      C: Facing vertically downwards  
D: Lying on the left side      E: Lying on the right side

This report is issued according to the general clauses in [www.ptc-testing.com](http://www.ptc-testing.com) by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted.  
The report could not be copied without permission

**Precise Testing & Certification (Guangdong) Co., Ltd. (PTC)**  
Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.  
Tel: 86-769-38808222      Fax: 86-769-38826111      [http:// www.ptc-testing.com](http://www.ptc-testing.com)



# Test Report

Report No.:PTC21030502102C-EN01

Issue Date:Apr.30, 2021

Page 8 of 13

Test	Uncertainty
Total inward leakage	3.8%
Penetration of filter material(NaCl)	3.5%
Penetration of filter material(Paraffin oil)	4.2%
Carbon dioxide content of the inhalation air	4.5%
Breathing resistance(30L/min)	5.2%
Breathing resistance(95L/min)	5.4%
Breathing resistance(160)L/min)	6.0%

Photo(s) of Sample:



This report is issued according to the general clauses in [www.ptc-testing.com](http://www.ptc-testing.com) by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted.  
The report could not be copied without permission

**Precise Testing & Certification (Guangdong) Co., Ltd. (PTC)**

Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.  
Tel: 86-769-38808222 Fax: 86-769-38826111 [http:// www.ptc-testing.com](http://www.ptc-testing.com)






# Test Report

Report No.:PTC21030502102C-EN01

Issue Date:Apr.30, 2021

Page 9 of 13

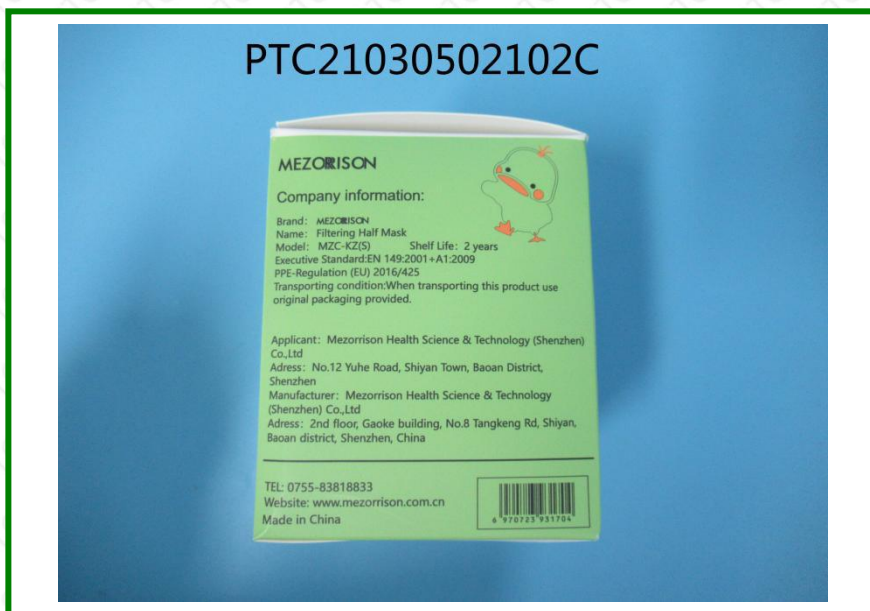

This report is issued according to the general clauses in [www.ptc-testing.com](http://www.ptc-testing.com) by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted.

The report could not be copied without permission

**Precise Testing & Certification (Guangdong) Co., Ltd. (PTC)**

Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.  
Tel: 86-769-38808222 Fax: 86-769-38826111 [http:// www.ptc-testing.com](http://www.ptc-testing.com)




# Test Report

Report No.:PTC21030502102C-EN01

Issue Date:Apr.30, 2021

Page 10 of 13

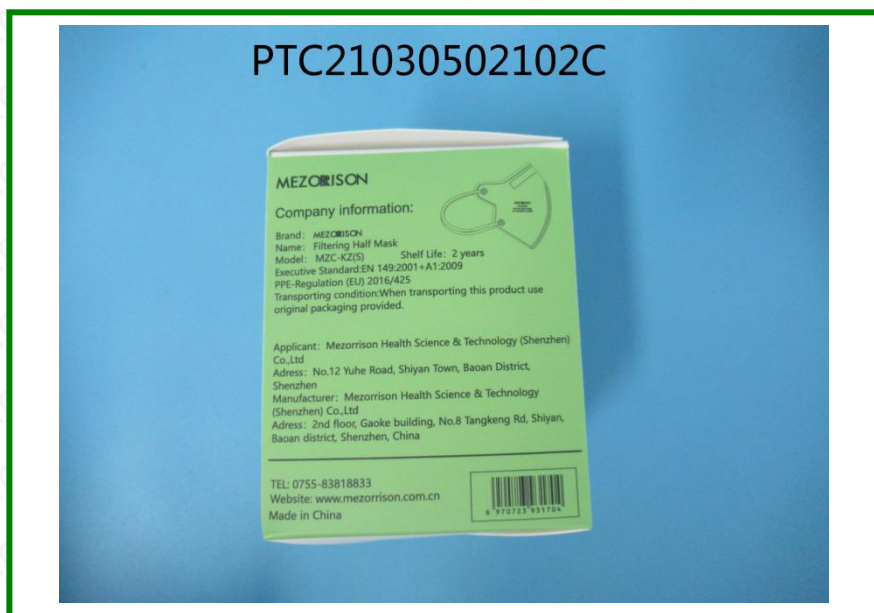

This report is issued according to the general clauses in [www.ptc-testing.com](http://www.ptc-testing.com) by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted.  
The report could not be copied without permission

**Precise Testing & Certification (Guangdong) Co., Ltd. (PTC)**  
Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.  
Tel: 86-769-38808222 Fax: 86-769-38826111 [http:// www.ptc-testing.com](http://www.ptc-testing.com)






# Test Report

Report No.:PTC21030502102C-EN01

Issue Date:Apr.30, 2021

Page 11 of 13

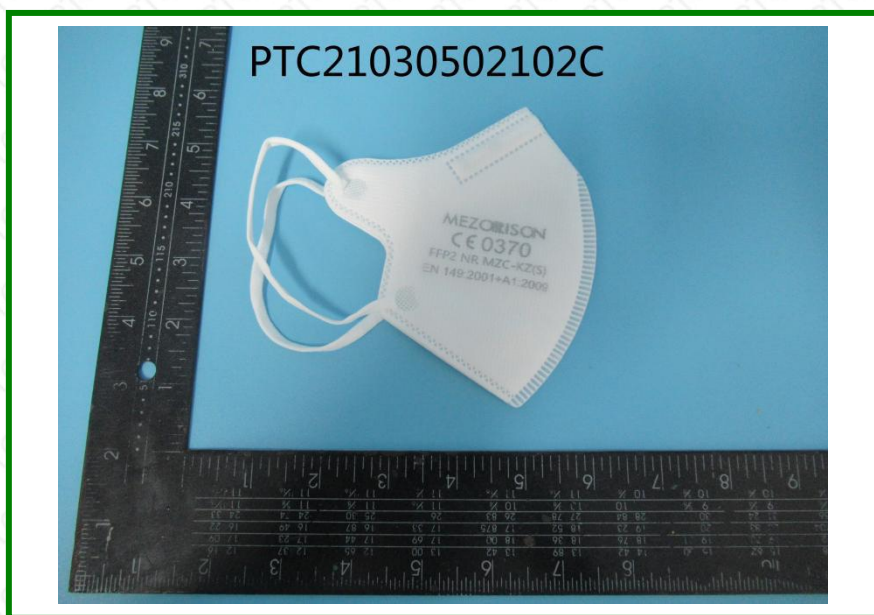

This report is issued according to the general clauses in [www.ptc-testing.com](http://www.ptc-testing.com) by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted. The report could not be copied without permission

**Precise Testing & Certification (Guangdong) Co., Ltd. (PTC)**  
Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.  
Tel: 86-769-38808222 Fax: 86-769-38826111 [http:// www.ptc-testing.com](http://www.ptc-testing.com)







# Test Report

Report No.:PTC21030502102C-EN01

Issue Date:Apr.30, 2021

Page 12 of 13

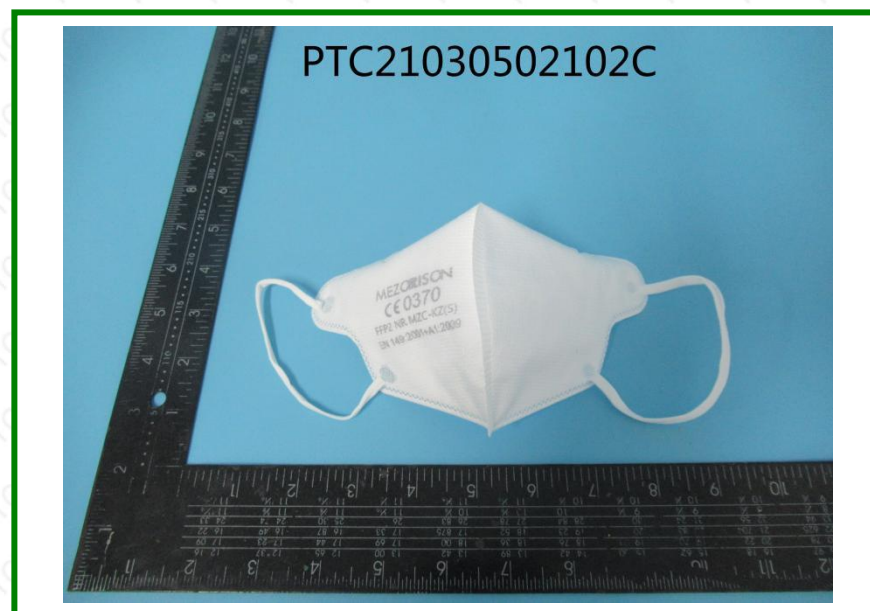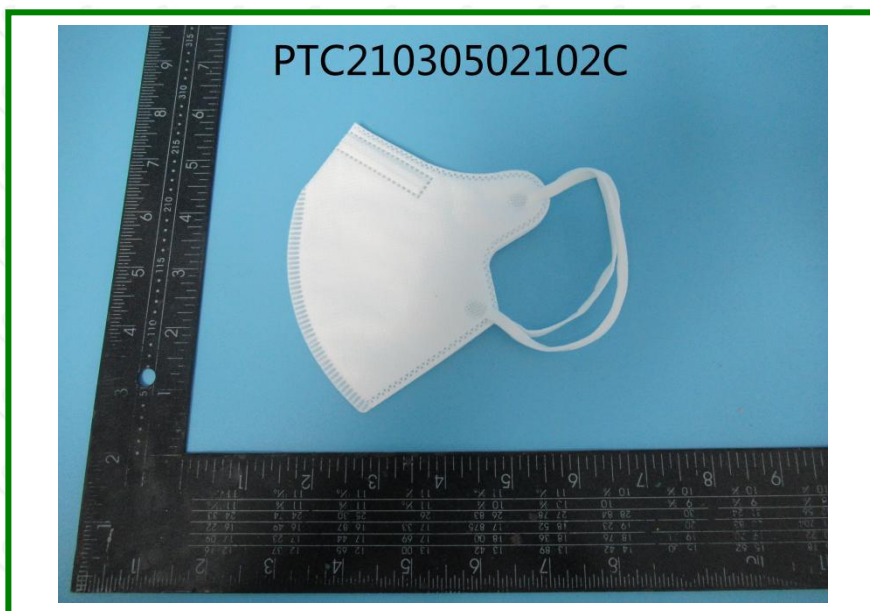

This report is issued according to the general clauses in [www.ptc-testing.com](http://www.ptc-testing.com) by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted.

The report could not be copied without permission

**Precise Testing & Certification (Guangdong) Co., Ltd. (PTC)**

Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.  
Tel: 86-769-38808222 Fax: 86-769-38826111 [http:// www.ptc-testing.com](http://www.ptc-testing.com)



# Test Report

Report No.:PTC21030502102C-EN01

Issue Date:Apr.30, 2021

Page 13 of 13



\*\*\*End of Report\*\*\*

This report is issued according to the general clauses in [www.ptc-testing.com](http://www.ptc-testing.com) by PTC. Responsibility, guarantee and law restriction are defined in the general service clauses. The report is only responsible for the submitted sample(s) except as otherwise noted.  
The report could not be copied without permission

**Precise Testing & Certification (Guangdong) Co., Ltd. (PTC)**

Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.  
Tel: 86-769-38808222 Fax: 86-769-38826111 [http:// www.ptc-testing.com](http://www.ptc-testing.com)